

Name: little 2, bird

OD



ID: 0000

Exam Date: 26/07/2021

CZMI

DOB: 1/07/2020

Exam Time: 5:10 PM

Gender: Unknown


Serial Number: 5000-5626

Technician: Operator, Cirrus



Signal Strength: N/A

Anterior Chamber Analysis : Anterior Chamber

OD OS

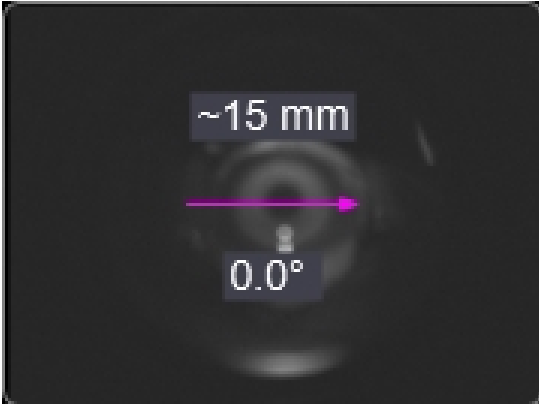

| Chamber Measurement | Value |
|---------------------|----------------------|
| Area | 8.49 mm ² |

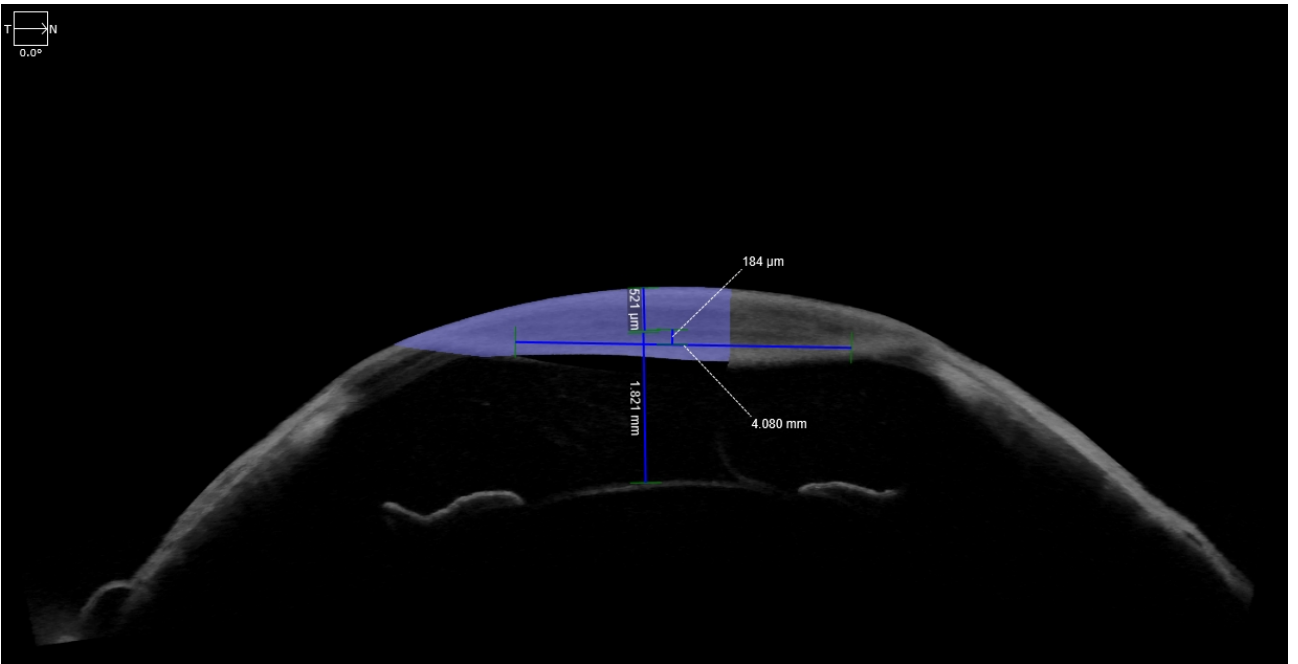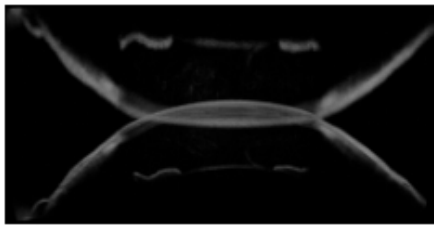

Comments

Analysis Edited: 1/10/2021 8:30 AM

Doctor's Signature

SW Ver: 11.5.2.54532
 Copyright 2020
 Carl Zeiss Meditec, Inc
 All Rights Reserved